

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING
Serial No. 10/787,307



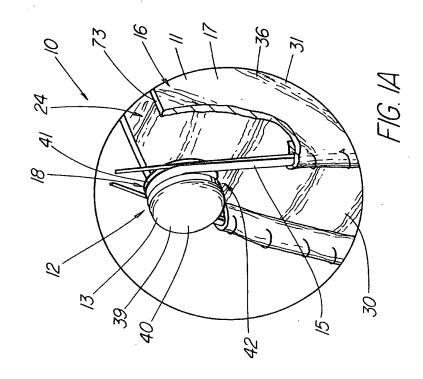

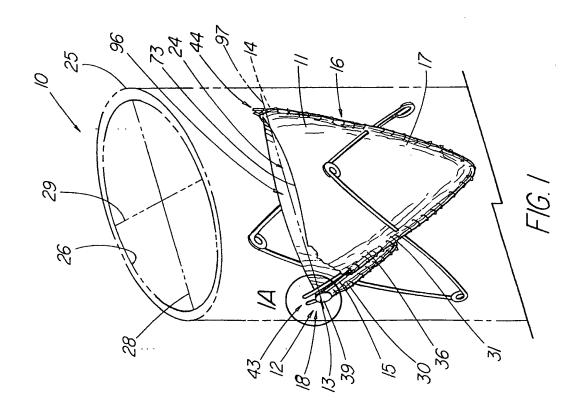

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING

Serial No. 10/787,307




FIG. 2


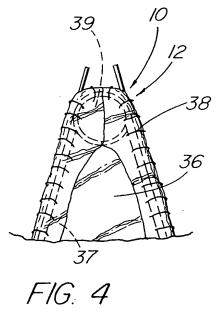


FIG. 3








FIG. 5

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING
Serial No. 10/787,307 3 of 8

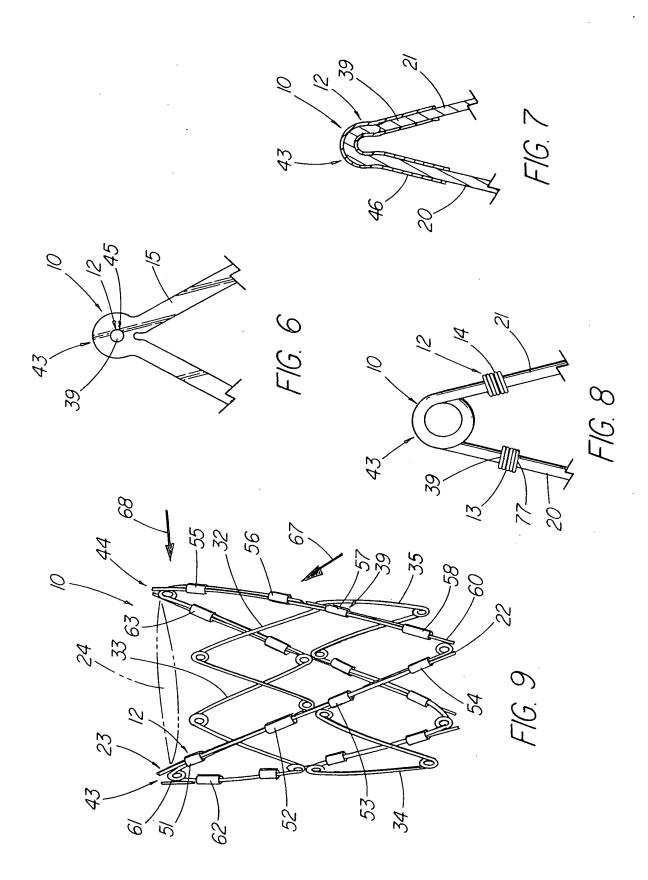



In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER EXTERNAL IMAGING

Serial No. 10/787,307

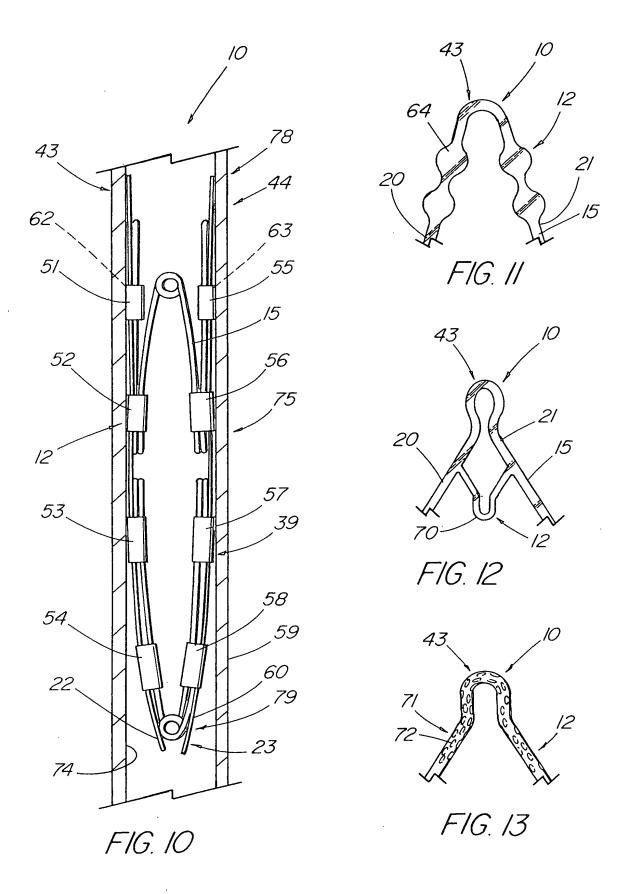




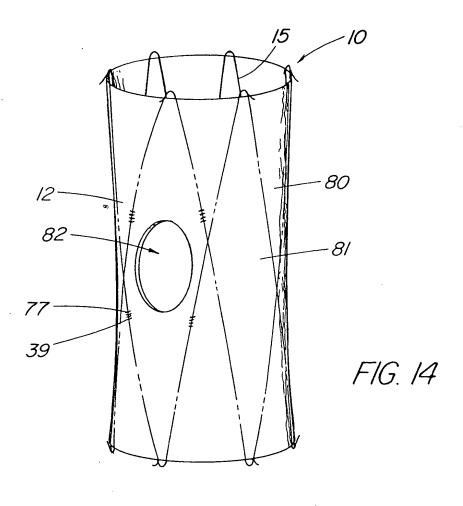

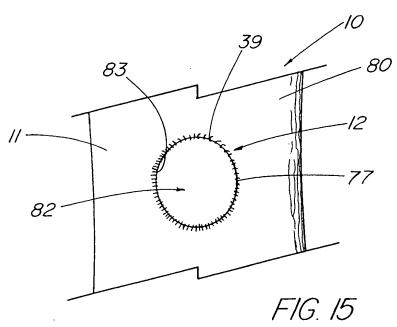


6 of 8


Serial No. 10/787,307

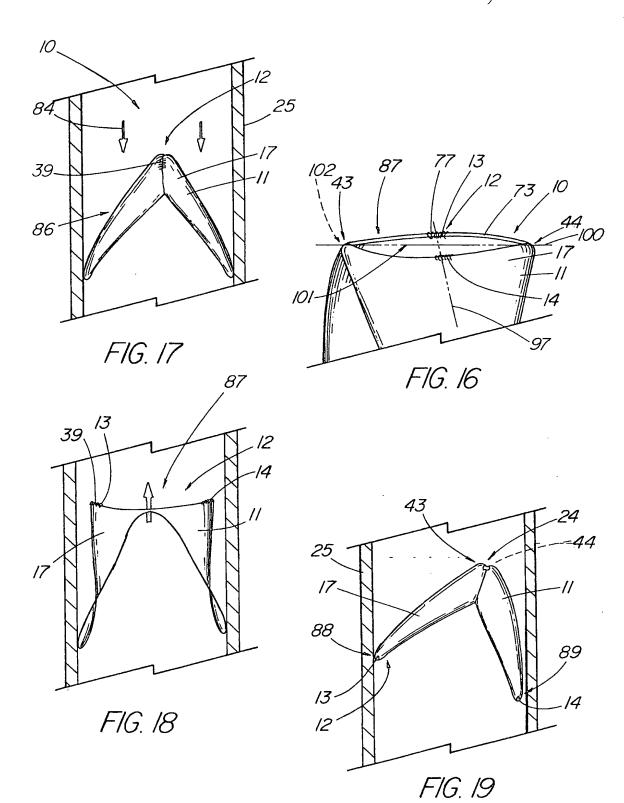

7 of 8

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING
Serial No. 10/787,307

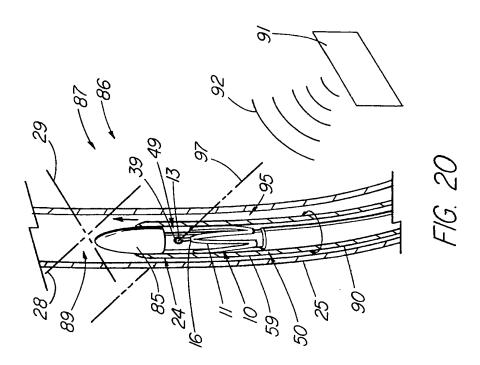

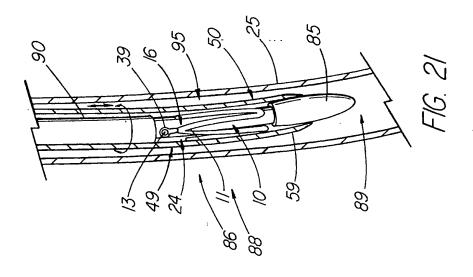

In RE: Case et al.
PROSTHESIS ADAPTED FOR PLACEMENT UNDER
EXTERNAL IMAGING
Serial No. 10/787,307

8 of 8

